

**IK4148 Human IL-12(p40) ELISA Kit**


- Size:** 96 T
- Range:** 31.2 pg/ml – 2000 pg/ml
- Sensitivity:** < 2 pg/ml
- Specificity:** No detectable cross-reactivity with any other cytokine.
- Applications:** For quantitative detection of human IGFBP-1 in sera, plasma, body fluids, tissue lysates or cell culture supernates.

Principle: Immunological Science's human IL-12(p40) ELISA Kit was based on standard sandwich enzyme-linked immune-sorbent assay technology. Human IL-12(p40) specific-specific monoclonal antibodies (clone No. 31052) were precoated onto 96-well plates. The human specific detection polyclonal antibodies were biotinylated. The test samples and biotinylated detection antibodies were added to the wells subsequently and then followed by washing with PBS or TBS buffer. Avidin-Biotin-Peroxidase Complex was added and unbound conjugates were washed away with PBS or TBS buffer. HRP substrate TMB was used to visualize HRP enzymatic reaction. TMB was catalyzed by HRP to produce a blue color product that changed into yellow after adding acidic stop solution. The density of yellow is proportional to the human IL-12(p40) amount of sample captured in plate.

Background: Interleukin-12 (IL12; formerly NKSF, for natural killer cell stimulatory factor, or CLMF, for cytotoxic lymphocyte maturation factor) is a novel cytokine cloned from B-cell lines. IL-12 is a heterodimeric molecule composed of p35 and p40 subunits. The larger 40-kDa subunit (p40) is a member of the cytokine receptor family, and the smaller 35-kDa subunit (p35) is related to IL6 and GCSF. Both IL-12 p40(-/-) and p35(-/-) mice fail to produce IL-12 p70 heterodimer. Interleukin (IL)-12 has been cloned on the basis of its ability to activate natural killer (NK) cells and promote the development of cytolytic T cells. With further understanding of its activities, IL-12 has emerged as an important cytokine, affecting both immune and hematologic functions. It has been shown to be necessary for the T cell independent induction of interferon (IFN)-gamma, critical for the initial suppression of bacterial and parasitic infection; for the development of a Th1 response, critical for effective host defense against intracellular pathogens; and for the activation of differentiated T lymphocytes of both CD4+ and CD8+ phenotype. The subunits map to different chromosomes: p40 (IL12B) to 5q31-q33 and p35 (IL12A) to 3p12-3q13.2. The standard product used in this kit is recombinant human IL-12(p40), which is a 40kDa glycoprotein consisting of 306 amino acids.

KIT COMPONENTS

1. Lyophilized recombinant human IL-12(p40) standard: 10ng/tube×2.
2. One 96-well plate precoated with anti- human IL-12(p40) antibody.
3. Sample diluent buffer: 30 ml
4. Biotinylated anti- human IL-12(p40) antibody : 130µl, dilution 1:100.
5. Antibody diluent buffer: 12ml.
6. Avidin-Biotin-Peroxidase Complex (ABC) : 130µl, dilution 1:100.
7. ABC diluent buffer: 12ml.
8. TMB color developing agent: 10ml.
9. TMB stop solution: 10ml.

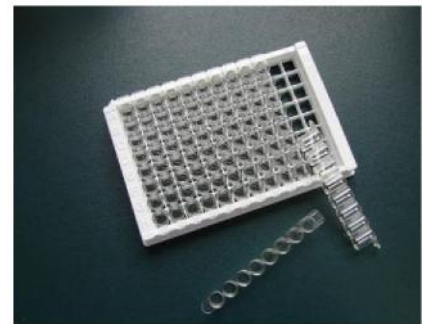

For Research use only; not for use as a diagnostic
IMMUNOLOGICAL SCIENCES

Web-site: www.immunologicalsciences.com

E-Mail: info@immunologicalsciences.com



IMMUNOLOGICAL SCIENCES

Product Data Sheet

Material Required But Not Provided

1. Microplate reader in standard size.
2. Automated plate washer.
3. Adjustable pipettes and pipette tips. Multichannel pipettes are recommended in the condition of large amount of samples in the detection.
4. Clean tubes and Eppendorf tubes.
5. Washing buffer (neutral PBS or TBS).
 - Preparation of 0.01M TBS: Add 1.2g Tris, 8.5g NaCl; 450µl of purified acetic acid or 700µl of concentrated hydrochloric acid to 1000ml H₂O and adjust pH to 7.2-7.6. Finally, adjust the total volume to 1L.
 - Preparation of 0.01 M PBS: Add 8.5g sodium chloride, 1.4g Na₂HPO₄ and 0.2g NaH₂PO₄ to 1000ml distilled water and adjust pH to 7.2-7.6.
 - Finally, adjust the total volume to 1L.

Notice for Application of Kit

1. Before using Kit, spin tubes and bring down all components to bottom of tube.
2. Duplicate well assay was recommended for both standard and sample testing.
3. Don't let 96-well plate dry, dry plate will inactivate active components on plate.
4. In order to avoid marginal effect of plate incubation due to temperature difference (reaction may be stronger in the marginal wells), it is suggested that the diluted ABC and TMB solution will be pre-warmed in 37°C for 30 min before using.

Storage : Store at 4°C for frequent use, at -20°C for infrequent use. Avoid multiple freeze-thaw cycles (Shipped with blue ice.)

Expiration: Four months at 4°C and eight months at -20°C

For Research use only; not for use as a diagnostic
IMMUNOLOGICAL SCIENCES

Web-site: www.immunologicalsciences.com

E-Mail: info@immunologicalsciences.com

Protocol for ELISA Kit

Human IL-12(p40) ELISA Kit

Preparation

- **Sample Preparation and Storage**

Store samples to be assayed within 24 hours at 2-8°C. For long-term storage, aliquot and freeze samples at -20°C. Avoid repeated freeze-thaw cycles.

- **Cell culture supernate, tissue lysate or body fluids:** Remove particulates by centrifugation, analyze immediately or aliquot and store at -20°C

Note: Bovine serum used in cell culture supernates may contain abundant IL-12(p40), avoiding using it.

- **Serum:** Allow the serum to clot in a serum separator tube (about 30 min) at room temperature. Centrifuge at approximately 1000 X g for 10 min. Analyze the serum immediately or aliquot and store frozen at -70°C.

- **Sample Dilution Guideline**

The user needs to estimate the concentration of the target protein in the sample and select a proper dilution factor so that the diluted target protein concentration falls near the middle of the linear regime in the standard curve. Dilute the sample using the provided diluent buffer. The following is a guideline for sample dilution. Several trials may be necessary in practice. **The sample must be well mixed with the diluents buffer.**

- **High target protein concentration (20-200ng/ml).** The working dilution is 1:100. i.e. Add 1 µl sample into 99 µl sample diluent buffer.
- **Medium target protein concentration (2-20ng/ml).** The working dilution is 1:10. i.e. Add 10 µl sample into 90 µl sample diluent buffer.
- **Low target protein concentration (31.2-2000pg/ml).** The working dilution is 1:2. i.e. Add 50 µl sample to 50 µl sample diluent buffer.
- **Very Low target protein concentration (≤31.2pg/ml).** No dilution necessary, or the working dilution is 1:2.

- **Reagent Preparation and Storage**

A. Reconstitution of the human IL-12(p40) standard: IL-12(p40) standard solution should be prepared no more than 2 hours prior to the experiment. Two tubes of IL-12(p40) standard (10ng per tube) are included in each kit. Use one tube for each experiment.

- 10,000pg/ml of human IL-12(p40) standard solution: Add 1 ml sample diluent buffer into one tube, keep the tube at room temperature for 10 min and mix thoroughly.
- 2000pg/ml of human IL-12(p40) standard solution: Add 0.2 ml of the above 10ng/ml IL-12(p40) standard solution into 0.8 ml sample diluent buffer and mix thoroughly.
- 1000pg/ml → 31.2pg/ml of human IL-12(p40) standard solutions: Label 6 Eppendorf tubes with 1000pg/ml, 500pg/ml, 250pg/ml, 125pg/ml, 62.5pg/ml, 31.2pg/ml, respectively. Aliquot 0.3 ml of the sample diluent buffer into each tube. Add 0.3 ml of the above 2000pg/ml IL-12(p40) standard solution into 1st tube and mix. Transfer 0.3 ml from 1st tube to 2nd tube and mix. Transfer 0.3 ml from 2nd tube to 3rd tube and mix, and so on.

Note: The standard solutions are best used within 2 hours. The 10ng/ml standard solution may be stored at 4°C for up to 12 hours, or at -20°C for up to 48 hours. Avoid repeated freeze-thaw cycles.

**For Research use only; not for use as a diagnostic
IMMUNOLOGICAL SCIENCES**

Web-site: www.immunologicalsciences.com

E-Mail: info@immunologicalsciences.com

Protocol for ELISA Kit

- B. Preparation of biotinylated anti-human IL-12(p40) antibody working solution: The solution should be prepared no more than 2 hours prior to the experiment.
- The total volume should be: 0.1ml/well x (the number of wells). (Allowing 0.1-0.2 ml more than total volume)
 - Biotinylated anti-human IL-12(p40) antibody should be diluted in 1:100 with the antibody diluent buffer and mixed thoroughly.
- C. Preparation of Avidin-Biotin-Peroxidase Complex (ABC) working solution: The solution should be prepared no more than 1 hour prior to the experiment.
- The total volume should be: 0.1ml/well x (the number of wells). (Allowing 0.1-0.2 ml more than total volume)
 - Avidin- Biotin-Peroxidase Complex (ABC) should be diluted in 1:100 with the ABC dilution buffer and mixed thoroughly.

Assay Procedure

The ABC working solution and TMB color developing agent must be kept warm at 37°C for 30 min before use. When diluting samples and reagents, they must be mixed completely and evenly. Standard IL-12(p40) detection curve should be prepared for each experiment. The user will decide sample dilution fold by crude estimation of IL-12(p40) amount in samples.

- Aliquot 0.1ml per well of the 2000pg/ml, 1000pg/ml, 500pg/ml, 250pg/ml, 125pg/ml, 62.5pg/ml, 31.2pg/ml human IL-12(p40) standard solutions into the precoated 96-well plate. Add 0.1ml of the sample diluent buffer into the control well (Zero well). Add 0.1ml of each properly diluted sample of human sera, plasma, body fluids, tissue lysates or cell culture supernatants to each empty well. **See “Sample Dilution Guideline” above for details.** We recommend that each human IL-12(p40) standard solution and each sample is measured in duplicate.
- Seal the plate with the cover and incubate at 37°C for 90 min.
- Remove the cover, discard plate content, and blot the plate onto paper towels or other absorbent material. Do NOT let the wells completely dry at any time.
- Add 0.1ml of biotinylated anti-human IL-12(p40) antibody working solution into each well and incubate the plate at 37°C for 60 min.
- Wash plate 3 times with 0.01M TBS or 0.01M PBS, and each time let washing buffer stay in the wells for 1 min. Discard the washing buffer and blot the plate onto paper towels or other absorbent material. (**Plate Washing Method:** Discard the solution in the plate without touching the side walls. Blot the plate onto paper towels or other absorbent material. Soak each well with at least 0.3 ml PBS or TBS buffer for 1~2 minutes. Repeat this process two additional times for a total of THREE washes. Note: For automated washing, aspirate all wells and wash THREE times with PBS or TBS buffer, overfilling wells with PBS or TBS buffer. Blot the plate onto paper towels or other absorbent material.)
- Add 0.1ml of prepared ABC working solution into each well and incubate the plate at 37°C in dark for 30 min.
- Wash plate 5 times with 0.01M TBS or 0.01M PBS, and each time let washing buffer stay in the wells for 1-2 min. Discard the washing buffer and blot the plate onto paper towels or other absorbent material. (See Step 5 for plate washing method).
- Add 90 µl of prepared TMB color developing agent into each well and incubate plate at 37°C for 15-20

**For Research use only; not for use as a diagnostic
IMMUNOLOGICAL SCIENCES**

Web-site: www.immunologicalsciences.com

E-Mail: info@immunologicalsciences.com

Protocol for ELISA Kit

min (**Note:** For reference only, the optimal incubation time should be determined by end user. And the shades of blue can be seen in the wells with the four most concentrated human IL-12(p40) standard solutions; the other wells show no obvious color).

9. Add 0.1ml of prepared TMB stop solution into each well. The color changes into yellow immediately.
10. Read the O.D. absorbance at 450nm in a microplate reader within 30 min after adding the stop solution.

For calculation, (the relative O.D.₄₅₀) = (the O.D.₄₅₀ of each well) – (the O.D.₄₅₀ of Zero well). The standard curve can be plotted as the relative O.D.₄₅₀ of each standard solution (Y) vs. the respective concentration of the standard solution (X). The human IL-12(p40) concentration of the samples can be interpolated from the standard curve.

Note: if the samples measured were diluted, multiply the dilution factor to the concentrations from interpolation to obtain the concentration before dilution.

Summary

1. Add samples and standards and incubate the plate at 37°C for 90 min. Do not wash.
2. Add biotinylated antibodies and incubate the plate at 37°C for 60 min. Wash plate 3 times with 0.01M TBS.
3. Add ABC working solution and incubate the plate at 37°C for 30 min. Wash plate 5 times with 0.01M TBS.
4. Add TMB color developing agent and incubate the plate at 37°C for 15-20 min.
5. Add TMB stop solution and read.


Typical Data Obtained from Human IL-12(p40)

(TMB reaction incubate at 37°C for 17 min)

Concentration	0.0pg/ml	31.2pg/ml	62.5pg/ml	125pg/ml	250pg/ml	500pg/ml	1000pg/ml	2000pg/ml
O.D.	0.024	0.096	0.163	0.310	0.559	1.161	1.890	2.883

Typical Human IL-12(p40) ELISA Kit Standard Curve

This standard curve was generated at IS for demonstration purpose only. A standard curve must be run with each assay.

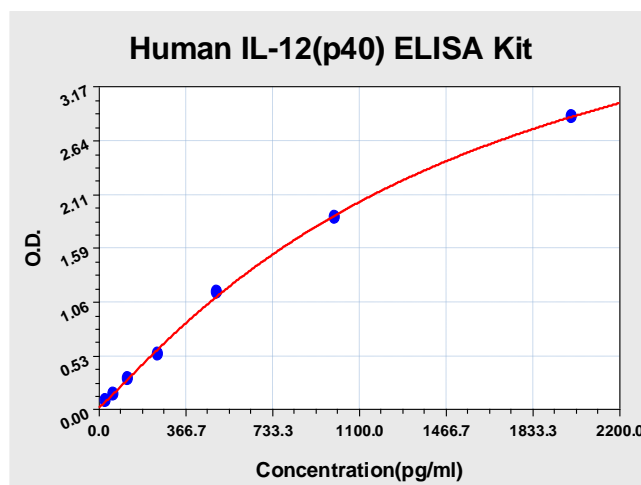

For Research use only; not for use as a diagnostic
IMMUNOLOGICAL SCIENCES

Web-site: www.immunologicalsciences.com

E-Mail: info@immunologicalsciences.com