

IK4182 Human TIMP-1 ELISA Kit

Size: 96T

Range: 15.6pg/ml-1000pg/ml

Sensitivity: < 5pg/ml

Specificity: No detectable cross-reactivity with any other cytokine.


Applications: For quantitative detection of human TIMP-1 in sera, plasma, body fluids, tissue lysates or cell culture supernates.

Principle: Immunological Sciences' human TIMP-1 ELISA Kit was based on standard sandwich enzyme-linked immune-sorbent assay technology. Human TIMP-1 specific-specific polyclonal antibodies were precoated onto 96-well plates. The human specific detection polyclonal antibodies were biotinylated. The test samples and biotinylated detection antibodies were added to the wells subsequently and then followed by washing with PBS or TBS buffer. Avidin-Biotin-Peroxidase Complex was added and unbound conjugates were washed away with PBS or TBS buffer. HRP substrate TMB was used to visualize HRP enzymatic reaction. TMB was catalyzed by HRP to produce a blue color product that changed into yellow after adding acidic stop solution. The density of yellow is proportional to the human TIMP-1 amount of sample captured in plate.

Background: The tissue inhibitor of metalloproteinases 1 (TIMP1) is also called erythroid-potentiating activity (EPA). The X-linked gene for human TIMP1 is expressed in some but not all inactive X-containing somatic-cell hybrids, suggesting that this gene is either prone to reactivation or variable in its inactivation.¹ Purified EPA specifically stimulates human and murine cells of the erythroid lineage, unlike murine interleukin-3 (IL-3) which stimulates precursor cells from all haematopoietic lineages.² TIMP1 is thought to play a regulatory role in connective tissues by forming inactive complexes with those metalloproteinases that are normally responsible for connective tissue turnover. The human gene encoding TIMP has been mapped to the X chromosome in the region Xp11.1-p11.4.³ The standard product used in this kit is natural TIMP-1 with the molecular mass of 22KDa.

KIT COMPONENTS

1. Lyophilized recombinant human TIMP-1 standard: 10ng/tubex2.
2. One 96-well plate precoated with anti- human TIMP-1 antibody.
3. Sample diluent buffer: 30 ml
4. Biotinylated anti- human TIMP-1 antibody : 130µl, dilution 1:100.
5. Antibody diluent buffer: 12ml.
6. Avidin-Biotin-Peroxidase Complex (ABC) : 130µl, dilution 1:100.
7. ABC diluent buffer: 12ml.
8. TMB color developing agent: 10ml.
9. TMB stop solution: 10ml.

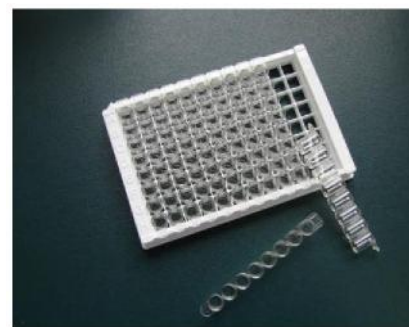

For Research use only; not for use as a diagnostic
IMMUNOLOGICAL SCIENCES

Web-site: www.immunologicalsciences.com

E-Mail: info@immunologicalsciences.com


Material Required But Not Provided

1. Microplate reader in standard size.
2. Automated plate washer.
3. Adjustable pipettes and pipette tips. Multichannel pipettes are recommended in the condition of large amount of samples in the detection.
4. Clean tubes and Eppendorf tubes.
5. Washing buffer (neutral PBS or TBS).
 - Preparation of 0.01M **TBS**: Add 1.2g Tris, 8.5g NaCl; 450µl of purified acetic acid or 700µl of concentrated hydrochloric acid to 1000ml H₂O and adjust pH to 7.2-7.6. Finally, adjust the total volume to 1L.
 - Preparation of 0.01 M **PBS**: Add 8.5g sodium chloride, 1.4g Na₂HPO₄ and 0.2g NaH₂PO₄ to 1000ml distilled water and adjust pH to 7.2-7.6. Finally, adjust the total volume to 1L.

Notice for Application of Kit

- 1 . Before using Kit, spin tubes and bring down all components to bottom of tube.
- 2 . Duplicate well assay was recommended for both standard and sample testing.
- 3 . Don't let 96-well plate dry, dry plate will inactivate active components on plate.
- 4 . In order to avoid marginal effect of plate incubation due to temperature difference (reaction may be stronger in the marginal wells), it is suggested that the diluted ABC and TMB solution will be pre-warmed in 37°C for 30 min before using.

Human TIMP-1 ELISA Kit-1X96 Well Plate Image

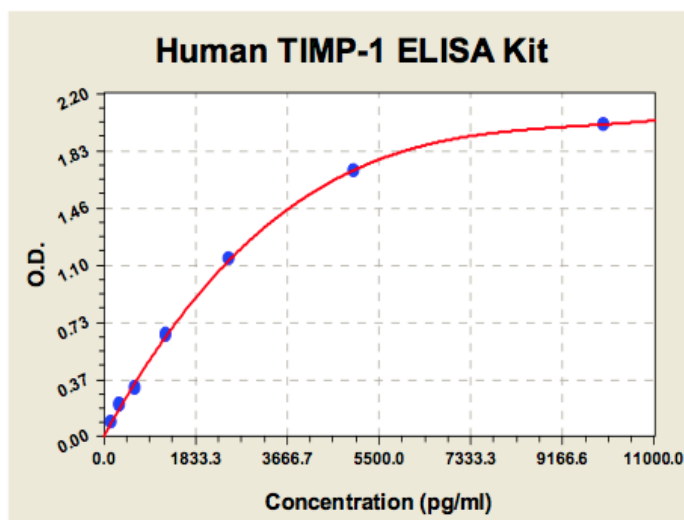

Storage Store at 4°C for frequent use, at -20°C for infrequent use. Avoid multiple freeze-thaw cycles (Shipped with wet ice.)

Expiration Four months at 4°C and eight months at -20°C.

For Research use only; not for use as a diagnostic

IMMUNOLOGICAL SCIENCES

Web-site: www.immunologicalsciences.com

E-Mail: info@immunologicalsciences.com